

Technical data sheet

miniRITE T

60 85 100 105



| | More 1 | More 2 | More 3 |
|--|--|--|--|
| Speech Understanding | | | |
| MoreSound Intelligence™ | Level 1 | Level 2 | Level 3 |
| - Environment configuration | 5 Options | 5 Options | 3 Options |
| - Virtual Outer Ear | 3 Configurations | 1 Configuration | 1 Configuration |
| - Spatial Balancer | 100% | 60% | 60% |
| - Neural Noise Suppression, Difficult / Easy | 10 dB / 4 dB | 6 dB / 2 dB | 6 dB / 0 dB |
| - Sound Enhancer | 3 Configurations | 2 Configurations | 1 Configuration |
| MoreSound Amplifier™ | • | • | • |
| Feedback Prevention | MoreSound Optimizer™ & Feedback shield | MoreSound Optimizer™ & Feedback shield | MoreSound Optimizer™ & Feedback shield |
| Spatial Sound™ | 4 Estimators | 2 Estimators | 2 Estimators |
| Soft Speech Booster | • | • | • |
| Frequency lowering | Speech Rescue™ | Speech Rescue™ | Speech Rescue™ |
| Sound Quality | | | |
| Clear Dynamics | • | • | - |
| Better-Ear Priority | • | • | - |
| Fitting Bandwidth | 10 kHz | 8 kHz | 8 kHz |
| Bass Boost (streaming) | • | • | • |
| Processing Channels | 64 | 48 | 48 |
| Listening Comfort | | | |
| Transient Noise Management | 4 configurations | 3 configurations | 3 configurations |
| Wind Noise Management | • | • | • |
| Personalisation & Optimising Fitting | | | |
| Fitting Bands | 24 | 20 | 18 |
| Multiple Directionality options | • | • | • |
| Adaptation Manager | • | • | • |
| Fitting Formulas | VAC+, NAL-NL1/ NAL-NL2, DSL 5.0 | VAC+, NAL-NL1/ NAL-NL2, DSL 5.0 | VAC+, NAL-NL1/ NAL-NL2, DSL 5.0 |
| Connecting to the world | | | |
| Stereo streaming (2.4 GHz) | • | • | • |
| Oticon ON app & Oticon RemoteCare app | • | • | • |
| ConnectClip | • | • | • |
| EduMic | • | • | • |
| Remote Control 3.0 | • | • | • |
| TV Adapter 3.0 | • | • | • |
| Phone Adapter 2.0 | • | • | • |
| Tinnitus SoundSupport™ | • | • | • |
| CROS / BiCROS support | • | • | • |

*Bandwidth accessible for gain adjustments during fitting

Operating Conditions

Temperature: +1°C to +40°C (34°F to 104°F)
 Humidity: 5% to 93% relative humidity, non-condensing
 Atmospheric pressure: 700 hPa to 1060 hPa

Storage and transportation conditions

Temperature and humidity should not exceed the below limits for extended periods during transportation and storage.

Transportation

Temperature: -25°C to +60°C (-13°F to 140°F)
 Humidity: 5% to 93% relative humidity, non-condensing
 Atmospheric pressure: 700 hPa to 1060 hPa

Storage

Temperature: -25°C to +60°C (-13°F to 140°F)
 Humidity: 5% to 93% relative humidity, non-condensing
 Atmospheric pressure: 700 hPa to 1060 hPa

Oticon More miniRITE T offers a discreet design with LED-light to make handling easy. The style features telecoil, and a double push button. It offers direct streaming from iPhone® and selected Android™ devices.

MoreSound Intelligence™ creates a more precise and natural representation of individual sounds with clearer and more distinct contrasts.

MoreSound Amplifier™ analyses details in sound, and optimally amplifies them for the brain to have access to relevant information.

Oticon More is built on the innovative Polaris™ platform, which uses a Deep Neural Network to rapidly and optimally manage incoming sounds based on individual needs. New features can be added and updated performed wirelessly.

General features:


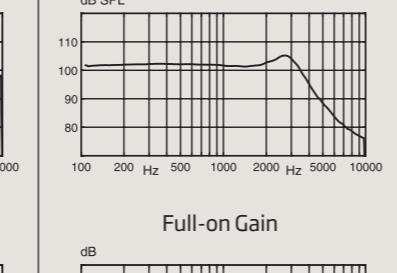







- Digital Programmable
- Automatic or Manual Volume Control
- Maximum Output Control System
- MPO-Maximum Power Output
- GC-Gain Control
- AGC-Automatic Gain Control
- Noise Reduction
- Feedback Management
- Dual Microphone
- FM Compatible (with Telecoil)
- 4 Programs

Apple, the Apple logo, iPhone, iPad, and iPod touch are trademarks of Apple Inc., registered in the U.S. and other countries.

For information on compatibility, please visit www.oticon.global/compatibility


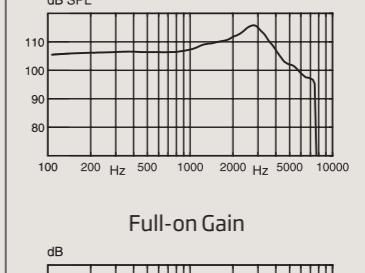

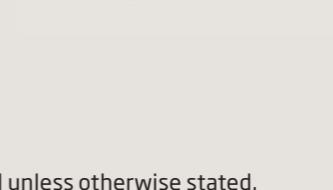




life-changing technology

Oticon More 1

| | | miniRITE T 60 | |
|---|---|---|---|
| | | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|  | 60 |  |  |
|  | OSPL90 |  | OSPL90 |
|  | Full-on Gain |  | Full-on Gain |
|  | Frequency Response |  | Frequency Response |
|  | Technical information Omnidirectional mode is used unless otherwise stated. |  | Technical information Omnidirectional mode is used unless otherwise stated. |
| | — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m | | — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m |
| OSPL90 | Peak 1600 Hz HFA-OSPL90 | 116 dB SPL 110 dB SPL 111 dB SPL | 105 dB SPL 102 dB SPL 103 dB SPL |
| Full-on gain* | Peak 1600 Hz HFA-FOG | 46 dB 37 dB 38 dB | 36 dB 29 dB 30 dB |
| Reference test gain | | 30 dB | 26 dB |
| Frequency range | | 100-9600 Hz | 100-9400 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field 10 mA/m field SPLITS L/R | 68 dB SPL 88 dB SPL - | - 85/85 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz 800 Hz 1600 Hz | <2 % <3 % <2 % | <2 % <2 % <2 % |
| Equivalent input noise level | Omni Dir | 18 dB SPL 26 dB SPL | 16 dB SPL 27 dB SPL |
| Battery consumption | Typical Quiescent | 2.3 mA 2.2 mA | 2.2 mA 2.2 mA |
| Battery life, artificial measurement, hours | | 80 | 80 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 55-60 | |



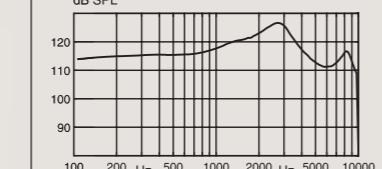

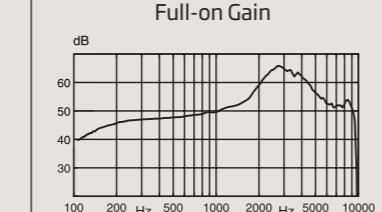

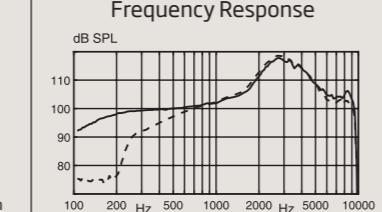

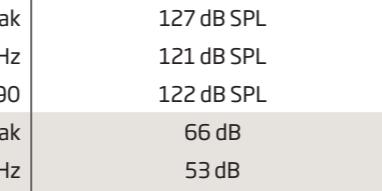

* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

Oticon More 2 & 3

| | | miniRITE T 60 | |
|--|---|---|---|
| | | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|  | 60 |  |  |
|  | OSPL90 |  | OSPL90 |
|  | Full-on Gain |  | Full-on Gain |
|  | Frequency Response |  | Frequency Response |
|  | Technical information Omnidirectional mode is used unless otherwise stated. |  | Technical information Omnidirectional mode is used unless otherwise stated. |
| | — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m | | — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m |
| OSPL90 | Peak 1600 Hz HFA-OSPL90 | 116 dB SPL 110 dB SPL 111 dB SPL | 105 dB SPL 102 dB SPL 103 dB SPL |
| Full-on gain* | Peak 1600 Hz HFA-FOG | 46 dB 37 dB 38 dB | 36 dB 29 dB 30 dB |
| Reference test gain | | 30 dB | 26 dB |
| Frequency range | | 100-7500 Hz | 100-7500 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field 10 mA/m field SPLITS L/R | 68 dB SPL 88 dB SPL - | - 85/85 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz 800 Hz 1600 Hz | <2 % <3 % <2 % | <2 % <2 % <2 % |
| Equivalent input noise level | Omni Dir | 18 dB SPL 26 dB SPL | 16 dB SPL 27 dB SPL |
| Battery consumption | Typical Quiescent | 2.2 mA 2.2 mA | 2.2 mA 2.2 mA |
| Battery life, artificial measurement, hours | | 80 | 80 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 55-60 | |







* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

Oticon More 1

| | | miniRITE T 85 | |
|---|--|---|---|
| | | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|  | 85 |  |  |
|  |  |  |  |
|  |  |  |  |
| OSPL90 | Peak 1600 Hz HFA-OSPL90 | 127 dB SPL 121 dB SPL 122 dB SPL | 117 dB SPL 113 dB SPL 114 dB SPL |
| Full-on gain* | Peak 1600 Hz HFA-FOG | 66 dB 53 dB 56 dB | 55 dB 45 dB 48 dB |
| Reference test gain | | 46 dB | 37 dB |
| Frequency range | | 100-9500 Hz | 100-8900 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field 10 mA/m field SPLITS L/R | 84 dB SPL 104 dB SPL - | - 96/96 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz 800 Hz 1600 Hz | <2 % <4 % <5 % | <2 % <2 % <2 % |
| Equivalent input noise level | Omni Dir | 21 dB SPL 29 dB SPL | 17 dB SPL 27 dB SPL |
| Battery consumption | Typical Quiescent | 2.4 mA 2.2 mA | 2.4 mA 2.2 mA |
| Battery life, artificial measurement, hours | | 75 | 75 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 50-60 | |

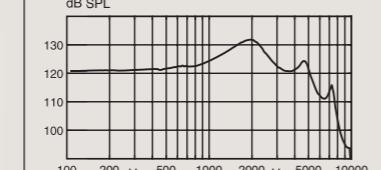
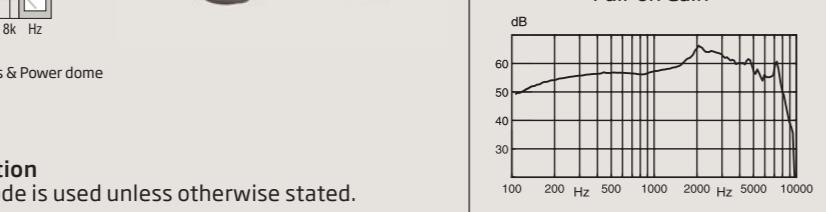

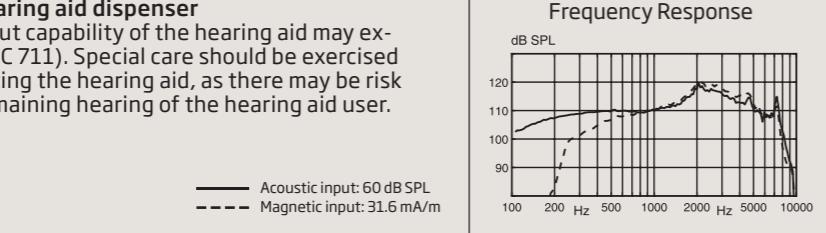

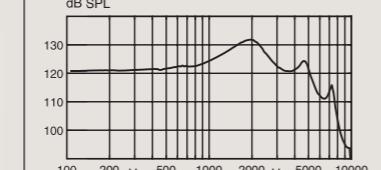
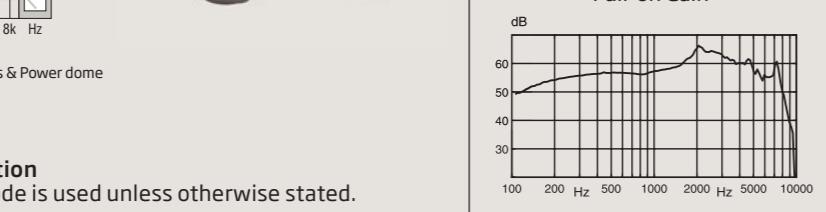

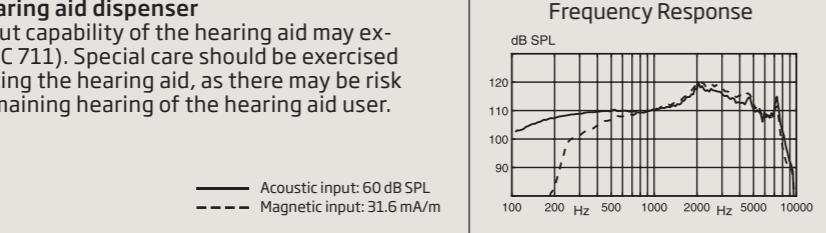


* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

Oticon More 2 & 3


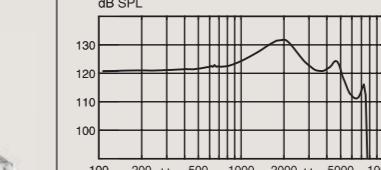
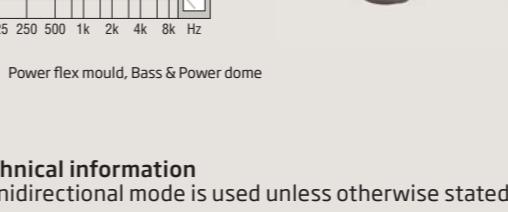
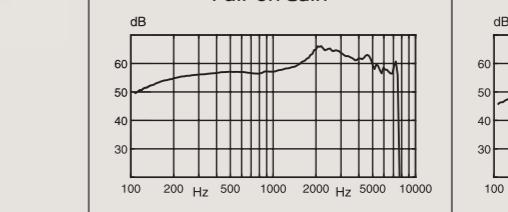
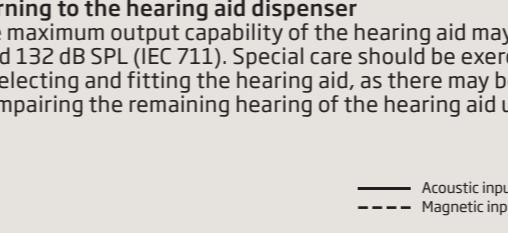
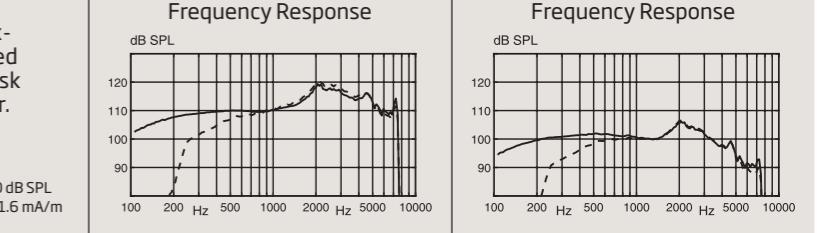

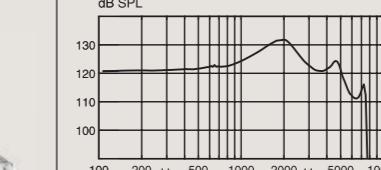
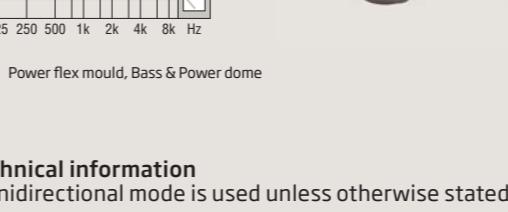
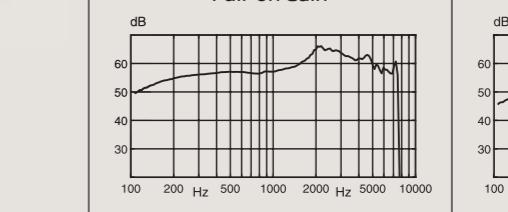
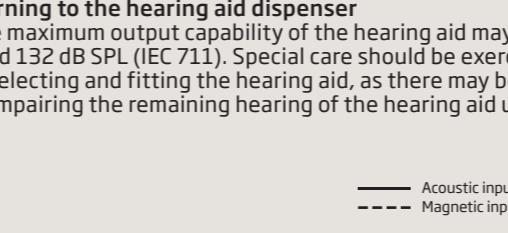
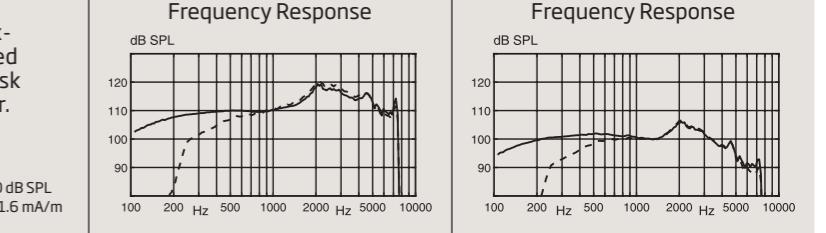


| | | miniRITE T 85 | |
|--|--|---|---|
| | | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|  | 85 |  |  |
|  |  |  |  |
|  |  |  |  |
| OSPL90 | Peak 1600 Hz HFA-OSPL90 | 127 dB SPL 121 dB SPL 122 dB SPL | 117 dB SPL 113 dB SPL 114 dB SPL |
| Full-on gain* | Peak 1600 Hz HFA-FOG | 66 dB 53 dB 56 dB | 55 dB 45 dB 48 dB |
| Reference test gain | | 46 dB | 37 dB |
| Frequency range | | 100-7500 Hz | 100-7500 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field 10 mA/m field SPLITS L/R | 84 dB SPL 104 dB SPL - | - 96/96 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz 800 Hz 1600 Hz | <2 % <4 % <5 % | <2 % <4 % <5 % |
| Equivalent input noise level | Omni Dir | 21 dB SPL 28 dB SPL | 17 dB SPL 27 dB SPL |
| Battery consumption | Typical Quiescent | 2.3 mA 2.2 mA | 2.4 mA 2.2 mA |
| Battery life, artificial measurement, hours | | 75 | 75 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 50-60 | |

* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

Oticon More 1

| | | miniRITE T 100 | |
|---|---|---|---|
| | | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|  | 100 |  OSPL90  OSPL90  Full-on Gain  Full-on Gain  Frequency Response  Frequency Response |  OSPL90  OSPL90  Full-on Gain  Full-on Gain  Frequency Response  Frequency Response |
|  | Power flex mould, Bass & Power dome |  | 100 |
| Technical information | Omnidirectional mode is used unless otherwise stated. | Technical information | Omnidirectional mode is used unless otherwise stated. |
| Warning to the hearing aid dispenser | The maximum output capability of the hearing aid may exceed 132 dB SPL (IEC 711). Special care should be exercised in selecting and fitting the hearing aid, as there may be risk of impairing the remaining hearing of the hearing aid user. | Warning to the hearing aid dispenser | The maximum output capability of the hearing aid may exceed 132 dB SPL (IEC 711). Special care should be exercised in selecting and fitting the hearing aid, as there may be risk of impairing the remaining hearing of the hearing aid user. |
| — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m | | — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m | |
| OSPL90 | Peak 1600 Hz HFA-OSPL90 | 132 dB SPL 130 dB SPL 127 dB SPL | 123 dB SPL 122 dB SPL 119 dB SPL |
| Full-on gain* | Peak 1600 Hz HFA-FOG | 66 dB 60 dB 61 dB | 57 dB 53 dB 53 dB |
| Reference test gain | | 53 dB | 42 dB |
| Frequency range | | 100-8900 Hz | 100-7500 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field 10 mA/m field SPLITS L/R | 91 dB SPL 111 dB SPL - | - 101/101 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz 800 Hz 1600 Hz | <9 % <6 % <3 % | <2 % <2 % <2 % |
| Equivalent input noise level | Omni Dir | 17 dB SPL 25 dB SPL | 16 dB SPL 28 dB SPL |
| Battery consumption | Typical Quiescent | 2.2 mA 2.2 mA | 2.4 mA 2.2 mA |
| Battery life, artificial measurement, hours | | 80 | 75 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 50-60 | |







Oticon More 2 & 3

| | | miniRITE T 100 | |
|---|---|--|--|
| | | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|  | 100 |  OSPL90  OSPL90  Full-on Gain  Full-on Gain  Frequency Response  Frequency Response |  OSPL90  OSPL90  Full-on Gain  Full-on Gain  Frequency Response  Frequency Response |
|  | Power flex mould, Bass & Power dome |  | 100 |
| Technical information | Omnidirectional mode is used unless otherwise stated. | Technical information | Omnidirectional mode is used unless otherwise stated. |
| Warning to the hearing aid dispenser | The maximum output capability of the hearing aid may exceed 132 dB SPL (IEC 711). Special care should be exercised in selecting and fitting the hearing aid, as there may be risk of impairing the remaining hearing of the hearing aid user. | Warning to the hearing aid dispenser | The maximum output capability of the hearing aid may exceed 132 dB SPL (IEC 711). Special care should be exercised in selecting and fitting the hearing aid, as there may be risk of impairing the remaining hearing of the hearing aid user. |
| — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m | | — Acoustic input: 60 dB SPL - - - Magnetic input: 31.6 mA/m | |
| OSPL90 | Peak 1600 Hz HFA-OSPL90 | 132 dB SPL 130 dB SPL 127 dB SPL | 123 dB SPL 122 dB SPL 119 dB SPL |
| Full-on gain* | Peak 1600 Hz HFA-FOG | 66 dB 60 dB 61 dB | 57 dB 53 dB 53 dB |
| Reference test gain | | 53 dB | 42 dB |
| Frequency range | | 100-7500 Hz | 100-7500 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field 10 mA/m field SPLITS L/R | 91 dB SPL 111 dB SPL - | - 101/101 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz 800 Hz 1600 Hz | <9 % <6 % <3 % | <2 % <2 % <2 % |
| Equivalent input noise level | Omni Dir | 16 dB SPL 25 dB SPL | 16 dB SPL 28 dB SPL |
| Battery consumption | Typical Quiescent | 2.2 mA 2.2 mA | 2.2 mA 2.2 mA |
| Battery life, artificial measurement, hours | | 80 | 75 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 50-60 | |

* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.






* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

Oticon More 1

| | 105 | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|--|---|--|--|
| OSPL90 |  | OSPL90 |  |
| Full-on Gain |  | Full-on Gain |  |
| Frequency Response |  | Frequency Response |  |
| Peak | 135 dB SPL | 127 dB SPL | |
| OSPL90 | 1600 Hz | 133 dB SPL | 126 dB SPL |
| | HFA-OSPL90 | 131 dB SPL | 123 dB SPL |
| Full-on gain* | Peak | 72 dB | 64 dB |
| | 1600 Hz | 66 dB | 59 dB |
| | HFA-FOG | 65 dB | 58 dB |
| Reference test gain | | 58 dB | 47 dB |
| Frequency range | | 100-9100 Hz | 100-7900 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field | 96 dB SPL | - |
| | 10 mA/m field | 116 dB SPL | - |
| | SPLITS L/R | - | 106/106 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz | < 4 % | < 2 % |
| | 800 Hz | < 4 % | < 2 % |
| | 1600 Hz | < 4 % | < 2 % |
| Equivalent input noise level | Omni | 15 dB SPL | 16 dB SPL |
| | Dir | 24 dB SPL | 27 dB SPL |
| Battery consumption | Typical | 2.3 mA | 2.4 mA |
| | Quiescent | 2.2 mA | 2.2 mA |
| Battery life, artificial measurement, hours | | 80 | 75 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 50-60 | |

miniRITE T 105

Oticon More 2 & 3

| | 105 | Ear Simulator Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2015, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010 | 2CC Coupler Measured according to ANSI S3.22-2014, IEC 60118-0:2015 and IEC 60318-5:2006 |
|--|--|--|--|
| OSPL90 |  | OSPL90 |  |
| Full-on Gain |  | Full-on Gain |  |
| Frequency Response |  | Frequency Response |  |
| Peak | 135 dB SPL | 127 dB SPL | 127 dB SPL |
| OSPL90 | 1600 Hz | 133 dB SPL | 126 dB SPL |
| | HFA-OSPL90 | 131 dB SPL | 123 dB SPL |
| Full-on gain* | Peak | 72 dB | 64 dB |
| | 1600 Hz | 66 dB | 59 dB |
| | HFA-FOG | 65 dB | 58 dB |
| Reference test gain | | 58 dB | 47 dB |
| Frequency range | | 100-7500 Hz | 100-7500 Hz |
| Telecoil output (1600 Hz) | 1 mA/m field | 96 dB SPL | - |
| | 10 mA/m field | 116 dB SPL | - |
| | SPLITS L/R | - | 106/106 dB SPL |
| Total harmonic distortion (Input 70 dB SPL) | 500 Hz | < 4 % | < 2 % |
| | 800 Hz | < 4 % | < 2 % |
| | 1600 Hz | < 4 % | < 2 % |
| Equivalent input noise level | Omni | 15 dB SPL | 16 dB SPL |
| | Dir | 24 dB SPL | 27 dB SPL |
| Battery consumption | Typical | 2.3 mA | 2.4 mA |
| | Quiescent | 2.2 mA | 2.2 mA |
| Battery life, artificial measurement, hours | | 80 | 75 |
| Expected battery life, hours (battery size 312 - IEC PR41) | | 50-60 | |

* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

* Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

miniRITE T 105

Notes

Notes

Headquarters
Oticon A/S
Kongebakken 9
DK-2765 Smørum
Denmark



SBO Hearing A/S
Kongebakken 9
DK-2765 Smørum
Denmark

241386TRUK/20210806/v1